


Instruction Manual

innoSens 125T

pH-Electrode for wastewater and desulfurization

Technical Data Sheet

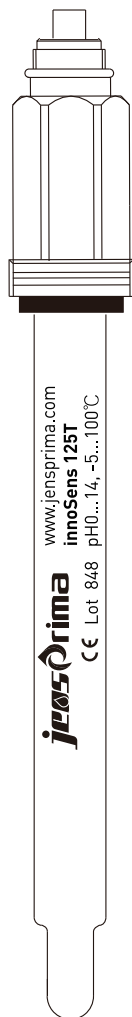

pH-Range:	pH 0...14
Temperature Range:	-5...100°C
Max.workingpressure:	6 bar
Shaft Material:	Glass
Electrolyte:	Polymer
Reference system:	Ag/AgCl cartridge
Diaphragm:	2 pore
Resistance:	≤300MΩ at 25°C
Diameter:	12 mm
Length:	120 mm
Membrane glass:	S-Glass
Temperature sensor:	PT 1000
Minimum immersion depth:	20 mm
Zero-Point:	0+/-20mV
Sensitivity:	57...59mV/pH at 25°C
Minimum conductivity of sample:	150 μS/cm
Reaction time:	pH 4..7 < 30s
connect:	PG13.5
Cabel:	5m

User manual electrodes

Electrode data at shipment

Test result are shown at the beginning of the German text



Complaints only with serial number and information about appeared error

Storage

- Upright in KCl with the connector head pointing upwards
- Temperature 10 to 30°C



Never store electrodes in deionized water, acids or lyes, this shortens the life time!

Installation

- Remove the protective cap
 - For liquid-filled electrodes also remove the black cap from the side connector and connect the KCl storage vessel.
- Make sure that the KCl level is always higher than the water level.
Always use 3M KCl for refill.



Install sensors upright with the connector head pointing upwards.



Threads PG 13.5 should be tightened hand-tight only.

Cable colors coding

Clear	pH
Shielding	Reference
Brown	PT1000(1)
White	PT1000(2)

Cleaning

- Rinse off wipe off loosely adherent dirt with a wet tissue
- For tenacious stains we recommend cleaning with diluted hydrochloric acid, organic pollutions can be removed with customary washing detergents
- To clean stained, blocked, or discoloured junctions use commercial cleaning solutions such as thiourea in diluted hydrochloric acid. Ceramic junctions can be abraded carefully.
- Rinse the electrode after every cleaning and store pH-sensors after cleaning for several hours in 3M KCl.



pH membranes and metal electrodes must not be cleaned mechanically!



At re-installation calibration is necessary (except ORP electrodes)